

KCMMM  
 #119  
 4727 E. Bell Rd.  
 STE 45  
 Phoenix  
 AZ  
 85032  
 (480) 586-4302  
 License #: AZ-T230007  
 Sample ID: 2310SMAZ0167.0461  
 Batch #: 10



**CERTIFICATE OF ANALYSIS**  
 License #: 00000020LCVT89602592

Certificate: 1043

## Hemp THCa Flower

Batch #: 10  
 Strain: 00007 Animal Cake  
 Parent Batch #:  
 Sample Collected:  
 Published: 10/30/2023

Sample ID: 2310SMAZ0167.0461  
 Amount Received: 5 g  
 Sample Type: Flower - Cured  
 Received: 10/18/2023

No Preview  
 Available

## COMPLIANCE FOR RETAIL

### Regulated Analytes

Cannabinoid Profile (Q3) <b>Tested</b>	Microbial Contaminants <b>Not Tested</b>	Residual Solvents <b>Not Tested</b>	<b>24.117%</b> Total THC
Pesticides, Fungicides, and Growth Regulators <b>Pass</b>	Mycotoxins <b>Not Tested</b>	Heavy Metals <b>Pass</b>	

### Additional Analytes (Not Regulated)


Terpenes Total (Q3) <b>Not Tested</b>	Moisture Analysis (Q3) <b>Not Tested</b>	Water Activity (Q3) <b>Not Tested</b>	<b>ND</b> CBN
Filth & Foreign (Q3) <b>Not Tested</b>	Homogeneity (Q3) <b>Not Tested</b>		<b>0.088%</b> CBG
			<b>27.970%</b> Total Cannabinoids (Q3)

Ahmed Munshi  
 Technical Laboratory Director

Smithers CTS Arizona LLC  
 734 W Highland Avenue, 2nd Floor  
 Phoenix, AZ 85013  
 (602) 806-6930



The product associated with this COA has been tested by Smithers CTS Arizona LLC, using validated state certified testing methodologies as required by Arizona state law. This COA is governed by the terms and conditions listed on: <https://www.smithers.com/arizona-terms-conditions>



KCMMM  
 #119  
 4727 E. Bell Rd.  
 STE 45  
 Phoenix  
 AZ  
 85032  
 (480) 586-4302  
 License #: AZ-T230007  
 Sample ID: 2310SMAZ0167.0461  
 Batch #: 10



**CERTIFICATE OF ANALYSIS**  
 License #: 00000020LCVT89602592

Certificate: 1043

**Cannabinoid Profile**

HPLC                      **Tested**

**Sample Prep**  
 Batch Date: 10/18/2023  
 SOP: 418.AZ  
 Batch Number: 184

**Sample Analysis**  
 Date: 10/20/2023  
 SOP: 417.AZ - HPLC  
 Sample Weight: 0.1023 g  
 Volume: 40 mL

Analyte	LOD (mg/g)	LOQ (mg/g)	Dil.	Actual % (w/w)	mg/g	Qualifier
CBC	0.126	0.382	1	<LOQ	<LOQ	
CBD	0.126	0.382	1	ND	ND	
CBDA	0.126	0.382	1	0.077	0.766	
CBDV	0.126	0.382	1	ND	ND	
CBG	0.126	0.382	1	0.088	0.881	
CBGA	0.126	0.382	1	0.497	4.975	
CBN	0.126	0.382	1	ND	ND	
d8-THC	0.126	0.382	1	ND	ND	
d9-THC	0.126	0.382	1	0.137	1.372	
THCA	0.126	0.382	1	25.936	259.359	
THCV	0.126	0.382	1	ND	ND	

Cannabinoid Totals	Actual % (w/w)	mg/g	Qualifier
Total THC	24.117	241.175	
Total CBD	0.067	0.672	
Total Cannabinoids	27.970	279.698	Q3


Total THC = THC + (0.877 x THCA) and Total CBD = CBD + (0.877 x CBDA)  
 ND = Not Detected, NT = Not Tested, <LOQ = Below Limit of Quantitation

**Ahmed Munshi**  
 Technical Laboratory Director

**Smithers CTS Arizona LLC**  
 734 W Highland Avenue, 2nd Floor  
 Phoenix, AZ 85013  
 (602) 806-6930



The product associated with this COA has been tested by Smithers CTS Arizona LLC, using validated state certified testing methodologies as required by Arizona state law. This COA is governed by the terms and conditions listed on: <https://www.smithers.com/arizona-terms-conditions>



KCMMM  
 #119  
 4727 E. Bell Rd.  
 STE 45  
 Phoenix  
 AZ  
 85032  
 (480) 586-4302  
 License #: AZ-T230007  
 Sample ID: 2310SMAZ0167.0461  
 Batch #: 10



**CERTIFICATE OF ANALYSIS**  
 License #: 00000020LCVT89602592

Certificate: 1043

**Heavy Metals**

ICP-MS **Pass**


**Sample Prep**

Batch Date: 10/19/2023  
 SOP: 428.AZ  
 Batch Number: 188

**Sample Analysis**

Date: 10/19/2023  
 SOP: 428.AZ - ICP-MS  
 Sample Weight: 0.2429 g  
 Volume: 6 mL

Analyte	LOD (ppm)	LOQ (ppm)	Dil.	Action Limit (ppm)	Results (ppm)	Qualifier
Arsenic	0.017	0.165	10	0.4	ND	
Cadmium	0.017	0.165	10	0.4	ND	
Lead	0.017	0.412	10	1	<LOQ	
Mercury	0.017	0.082	10	0.2	ND	

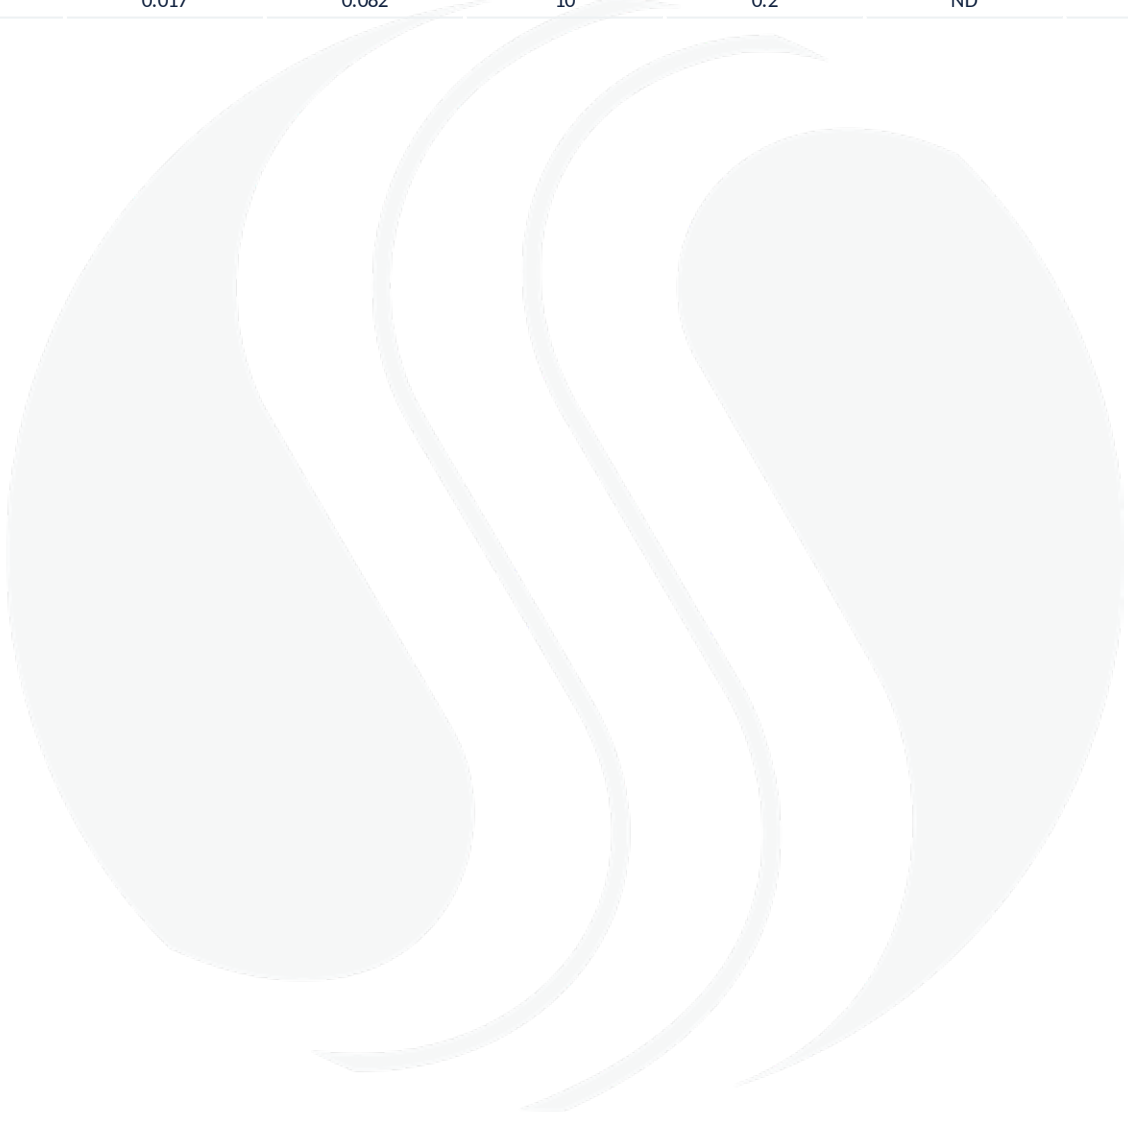

**Ahmed Munshi**


Technical Laboratory Director

**Smithers CTS Arizona LLC**  
 734 W Highland Avenue, 2nd Floor  
 Phoenix, AZ 85013  
 (602) 806-6930



Accreditation #: 103104

The product associated with this COA has been tested by Smithers CTS Arizona LLC, using validated state certified testing methodologies as required by Arizona state law. This COA is governed by the terms and conditions listed on: <https://www.smithers.com/arizona-terms-conditions>



KCMMM  
 #119  
 4727 E. Bell Rd.  
 STE 45  
 Phoenix  
 AZ  
 85032  
 (480) 586-4302  
 License #: AZ-T230007  
 Sample ID: 2310SMAZ0167.0461  
 Batch #: 10



**CERTIFICATE OF ANALYSIS**  
 License #: 00000020LCVT89602592

Certificate: 1043

**Pesticides, Fungicides, and  
 Growth Regulators**  
 LC-MS/MS **Pass**

**Sample Prep**

Batch Date: 10/18/2023  
 SOP: 432.AZ  
 Batch Number: 178

**Sample Analysis**

Date: 10/19/2023  
 SOP: 424.AZ - LC-MS/MS  
 Sample Weight: 0.5025 g  
 Volume: 12.5 mL

Analyte	LOD / LOQ (ppm)	Dil.	Action Limit (ppm)	Results (ppm)	Qualifier	Analyte	LOD / LOQ (ppm)	Dil.	Action Limit (ppm)	Results (ppm)	Qualifier
Abamectin B1a	0.083 / 0.249	1	0.5	ND	I1	Hexythiazox	0.166 / 0.498	1	1	ND	M2
Acephate	0.067 / 0.199	1	0.4	ND		Imazalil	0.033 / 0.100	1	0.2	ND	
Acetamiprid	0.033 / 0.100	1	0.2	ND		Imidacloprid	0.067 / 0.199	1	0.4	ND	
Aldicarb	0.067 / 0.199	1	0.4	ND		Kresoxim-methyl	0.067 / 0.199	1	0.4	ND	
Azoxystrobin	0.033 / 0.100	1	0.2	ND		Malathion	0.033 / 0.100	1	0.2	ND	
Bifenazate	0.033 / 0.100	1	0.2	ND		Metaxyl	0.033 / 0.100	1	0.2	ND	
Bifenthrin	0.033 / 0.100	1	0.2	ND	M2	Methiocarb	0.033 / 0.100	1	0.2	ND	M1
Boscalid	0.067 / 0.199	1	0.4	ND	M1	Methomyl	0.067 / 0.199	1	0.4	ND	
Carbaryl	0.033 / 0.100	1	0.2	ND		Myclobutanil	0.033 / 0.100	1	0.2	ND	M1
Carbofuran	0.033 / 0.100	1	0.2	ND		Naled	0.083 / 0.249	1	0.5	ND	
Chlorantraniliprole	0.033 / 0.100	1	0.2	ND	M1	Oxamyl	0.166 / 0.498	1	1	ND	
Chlorfenapyr	0.166 / 0.498	1	1	ND	I1, M1	Pacllobutrazol	0.067 / 0.199	1	0.4	ND	M1
Chlorpyrifos	0.033 / 0.100	1	0.2	ND	M2	Permethrins	0.033 / 0.100	1	0.2	ND	I1, M2
Clofentezine	0.033 / 0.100	1	0.2	ND		Phosmet	0.033 / 0.100	1	0.2	ND	
Cyfluthrin	0.166 / 0.498	1	1	ND		Piperonyl Butoxide	0.331 / 0.995	1	2	ND	M2
Cypermethrin	0.166 / 0.498	1	1	ND	M2	Prallethrin	0.033 / 0.100	1	0.2	ND	
Daminozide	0.166 / 0.498	1	1	ND		Propiconazole	0.067 / 0.199	1	0.4	ND	
Diazinon	0.033 / 0.100	1	0.2	ND		Propoxur	0.033 / 0.100	1	0.2	ND	
Dichlorvos	0.017 / 0.050	1	0.1	ND		Pyrethrins	0.139 / 0.417	1	1	ND	I1, M1
Dimethoate	0.033 / 0.100	1	0.2	ND		Pyridaben	0.033 / 0.100	1	0.2	ND	M2
Ethoprophos	0.033 / 0.100	1	0.2	ND		Spinosad	0.033 / 0.100	1	0.2	ND	M2
Etofenprox	0.067 / 0.199	1	0.4	ND		Spiromesifen	0.033 / 0.100	1	0.2	ND	
Etoxazole	0.033 / 0.100	1	0.2	ND		Spirotetramat	0.033 / 0.100	1	0.2	ND	
Fenoxycarb	0.033 / 0.100	1	0.2	ND		Spiroxamine	0.067 / 0.199	1	0.4	ND	
Fenpyroximate	0.067 / 0.199	1	0.4	ND	M2	Tebuconazole	0.067 / 0.199	1	0.4	ND	
Fipronil	0.067 / 0.199	1	0.4	ND		Thiacloprid	0.033 / 0.100	1	0.2	ND	
Fonicamid	0.166 / 0.498	1	1	ND		Thiamethoxam	0.033 / 0.100	1	0.2	ND	
Fludioxonil	0.067 / 0.199	1	0.4	ND	M1	Trifloxystrobin	0.033 / 0.100	1	0.2	ND	M2


**Ahmed Munshi**  
 Technical Laboratory Director

*Ahmed Munshi*

**Smithers CTS Arizona LLC**  
 734 W Highland Avenue, 2nd Floor  
 Phoenix, AZ 85013  
 (602) 806-6930



The product associated with this COA has been tested by Smithers CTS Arizona LLC, using validated state certified testing methodologies as required by Arizona state law. This COA is governed by the terms and conditions listed on: <https://www.smithers.com/arizona-terms-conditions>



KCMMM  
 #119  
 4727 E. Bell Rd.  
 STE 45  
 Phoenix  
 AZ  
 85032  
 (480) 586-4302  
 License #: AZ-T230007  
 Sample ID: 2310SMAZ0167.0461  
 Batch #: 10

Certificate: 1043



**CERTIFICATE OF ANALYSIS**  
 License #: 00000020LCVT89602592

## Qualifier Legend

- B1** The target analyte detected in the calibration is at or above the limit of quantitation, but the sample result for potency testing, is below the limit of quantitation.
- B2** The target analyte detected in the calibration blank, or the method blank is at or above the limit of quantitation, but the sample result when testing for pesticides, fungicides, herbicides, growth regulators, heavy metals, or residual solvents, is below the maximum allowable concentration for the analyte.
- D1** The limit of quantitation and the sample results were adjusted to reflect sample dilution.
- I1** The relative intensity of a characteristic ion in a sample analyte exceeded the acceptance with respect to the reference spectra, indicating interference.
- L1** When testing for pesticides, fungicides, herbicides, growth regulators, heavy metals, or residual solvents, the percent recovery of a laboratory control sample is greater than the acceptance limits, but the sample's target analytes were not detected above the maximum allowable concentrations for the analytes in the sample.
- M1** The recovery from the matrix spike was high, but the recovery from the laboratory control sample was within acceptance criteria.
- M2** The recovery from the matrix spike was low, but the recovery from the laboratory control sample was within acceptance criteria.
- M3** The recovery from the matrix spike was unusable because the analyte concentration was disproportionate to the spike level, but the recovery from the laboratory control sample was within acceptance criteria.
- M4** The analysis of a spiked sample required a dilution such that the spike recovery calculation does not provide useful information, but the recovery from the associated laboratory control sample was within acceptance criteria.
- M5** The analyte concentration was determined by the method of standard addition, in which the standard is added directly to the aliquots of the analyzed sample.
- M6** A description of the variance is described in the final report of testing according to R9-17- 404.06(B)(3)(d)(ii).
- Q1** Sample integrity was not maintained.
- Q2** The sample is heterogeneous, and sample homogeneity could not be readily achieved using routine laboratory practices.
- Q3** Testing result is for informational purposes only and cannot be used to satisfy dispensary testing requirements in R9-17-317.01(A) or labeling requirements in R9-17-317.
- R1** The relative percent difference for the laboratory control sample and duplicate exceeded the limit, but the recovery was within acceptance criteria.
- R2** The relative percent difference for a sample and duplicate exceeded the limit.
- V1** The recovery from continuing calibration verification standards exceeded the acceptance limits, but the sample's target analytes were not detected above the maximum allowable for the analytes in the sample.

## Notes:

Ahmed Munshi

Technical Laboratory Director

Smithers CTS Arizona LLC  
 734 W Highland Avenue, 2nd Floor  
 Phoenix, AZ 85013  
 (602) 806-6930



Accreditation #: 103104

The product associated with this COA has been tested by Smithers CTS Arizona LLC, using validated state certified testing methodologies as required by Arizona state law. This COA is governed by the terms and conditions listed on: <https://www.smithers.com/arizona-terms-conditions>